




## OPERATING INSTRUCTIONS

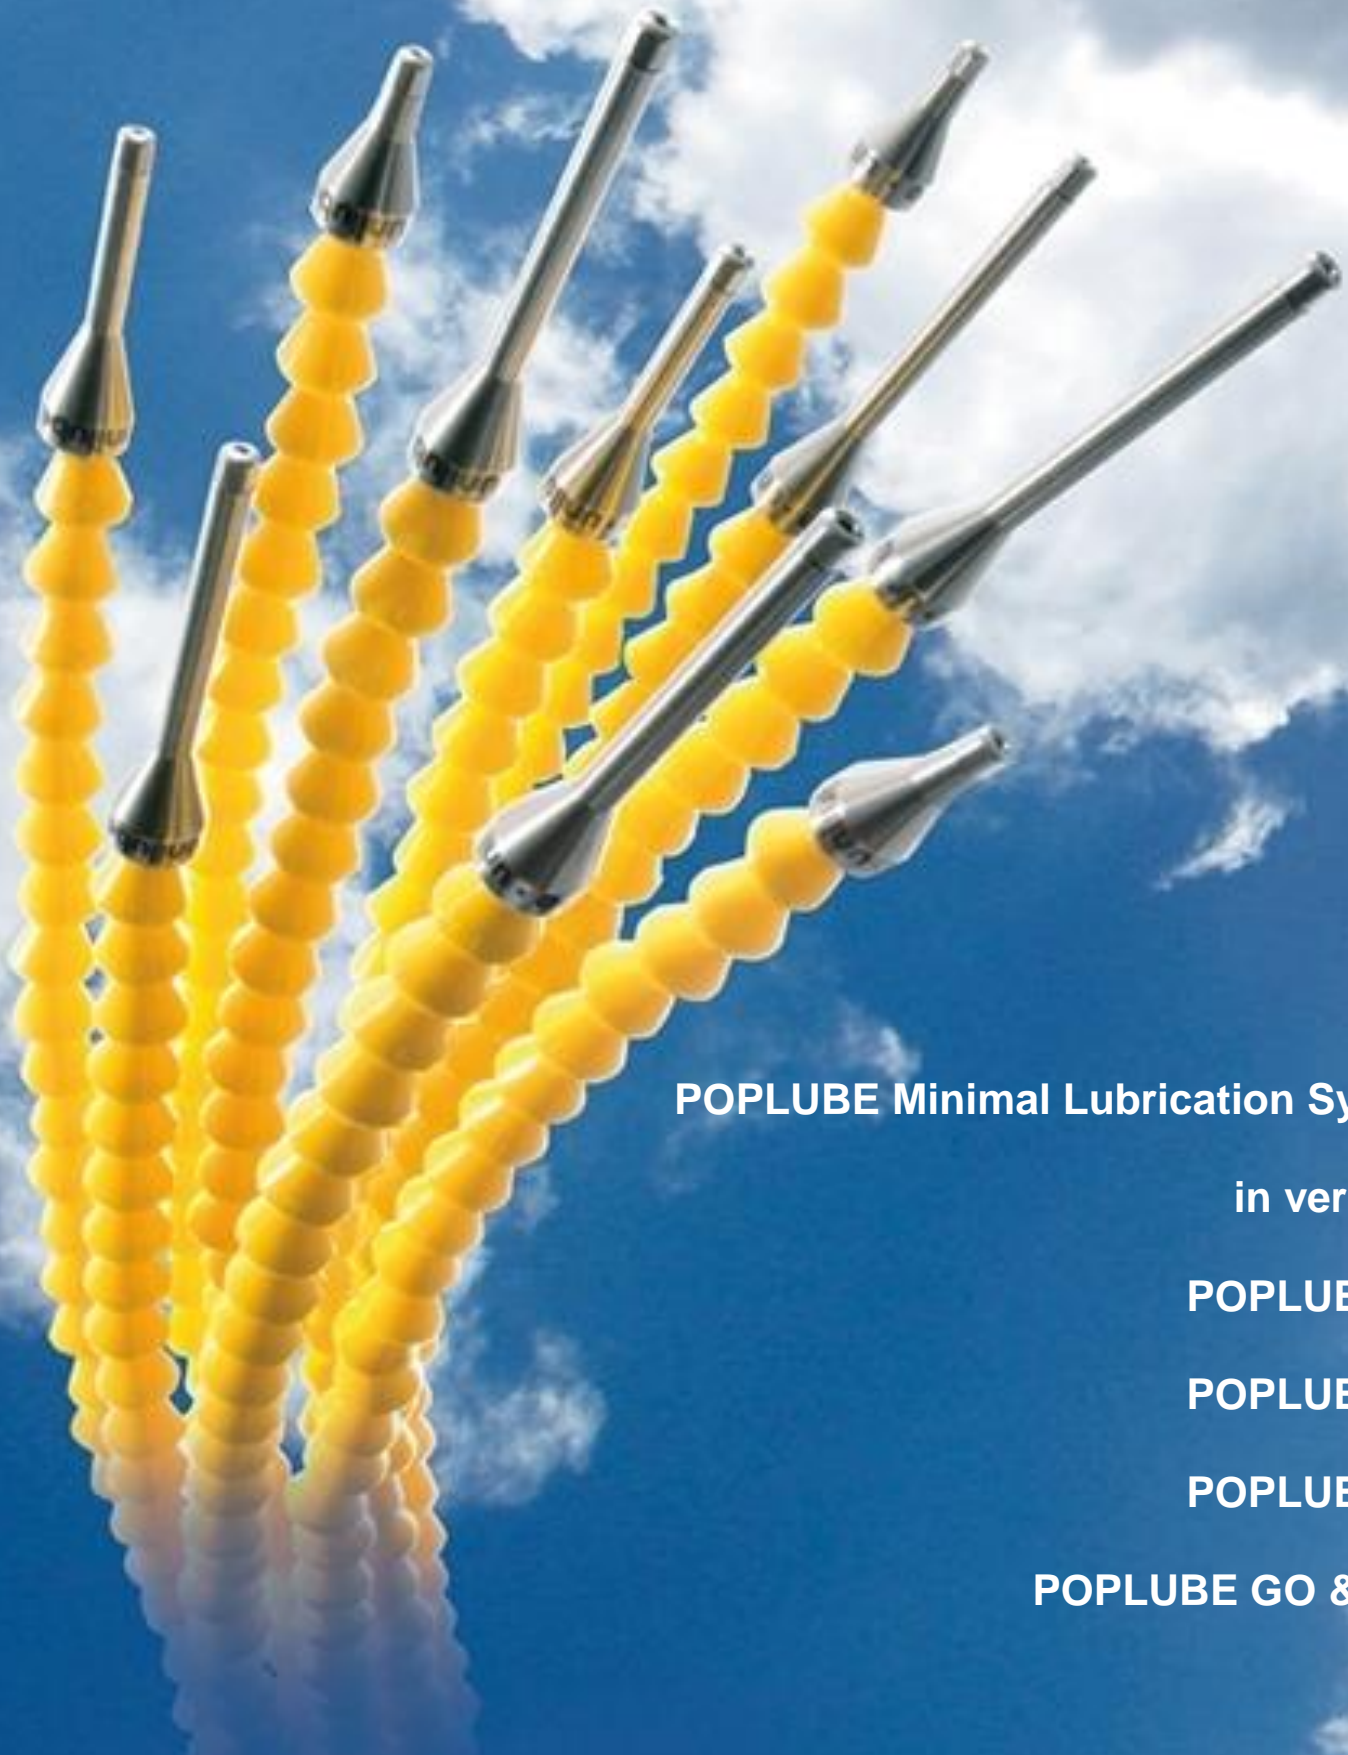

**POPLUBE Minimal Lubrication System**

**in versions**

**POPLUBE 1D**

**POPLUBE 2D**

**POPLUBE 3D**

**POPLUBE GO & FOX**

Table of contents

	Page
0. General information .....	3
1. Field of application and general safety instructions .....	4
2. Environmental regulations .....	5
3. Composition .....	6
4. Structure, mounting and connection .....	8
5. Filling with high-performance lubricant and operating conditions .....	12
6. Setting tasks .....	14
7. Factory settings .....	16
8. Venting, maintenance and cleaning .....	17
9. Start-up summary .....	19
10. Lubricant consumption values .....	20
11. Supplementary documentation .....	22
12. Abbreviations used .....	23



Quick start-up:

SEE Chapter 9



Important note:

LAYOUT, TECHNICAL SPECIFICATIONS, SAFETY DATA SHEETS and HIGH-PERFORMANCE LUBRICANT INFORMATION SHEET are part of the OPERATING INSTRUCTIONS.

## 0. General information

### 0.1 Manufacturing and sales



UNILUBE LTD - MICRO LUBRICATION TECHNOLOGY  
ANDHAUSERSTRASSE 52 A - CH-8572 BERG / TG  
TEL + 41-71 672 65 22 - FAX + 41-71 672 65 32  
[www.unilube.ch](http://www.unilube.ch) - [info@unilube.ch](mailto:info@unilube.ch)



Fig. 1: POPLUBE Minimal Lubrication System Version 1D with option main control valve with LED socket

## 1. Field of application and general safety instructions

- 1.1 The Minimal Lubrication System (MLS) is designed exclusively for applying a minimum quantity of lubricant (MQL) to a spatially limited point of need (e.g. tool, workpiece, bearing).
- 1.2 Specific warnings and operating instructions for the use of the MLS are given in the chapters of the operating instructions; these are marked with the following symbols and must be observed:



General warning / Important note



Fire / explosion hazard



Danger from electricity



Eye protection



**Important note:**

**The Minimal Lubrication System must not be started until it has been established that it has been connected in accordance with the operating instructions and associated specifications and that the machine and MLS are in a safe operating condition.**

**The manufacturer is not liable for damage to or caused by the Minimal Lubrication System resulting from improper installation or use, for example due to unsuitable equipment or settings.**

**Injury to people or damage to the MLS or the machine can occur due to lack of care or improper working methods; the operator is liable for this injury or damage.**

## 2. Environmental regulations and "Greta"

- 2.1 The Minimal Lubrication System does not contain any components that fall under the restrictions of the REACH and RoHS directives and is manufactured so that it is CE compliant.



- 2.2 Correct use of the UNILUBE Minimal Lubrication System ensures that environmentally friendly consumption with highly efficient performance can be achieved because the quantity of lubricant can be matched exactly to requirements. For this purpose, it is absolutely essential that the information in the operating instructions, the technical specifications and information sheets is followed.

Incorrect metering leads to increased consumption, as well as lower performance, and harms the environment.

- 2.3 The raw materials used in the Minimum Lubrication System are recyclable:

- aluminium, untreated
- stainless steels
- brass
- plastics, PA, PU, NBR



- 2.4 When decommissioning and disposing of the MLS at end of life, national regulations must be observed.



### 3. Composition: Illustration of POPLUBE 2D with equipment variants

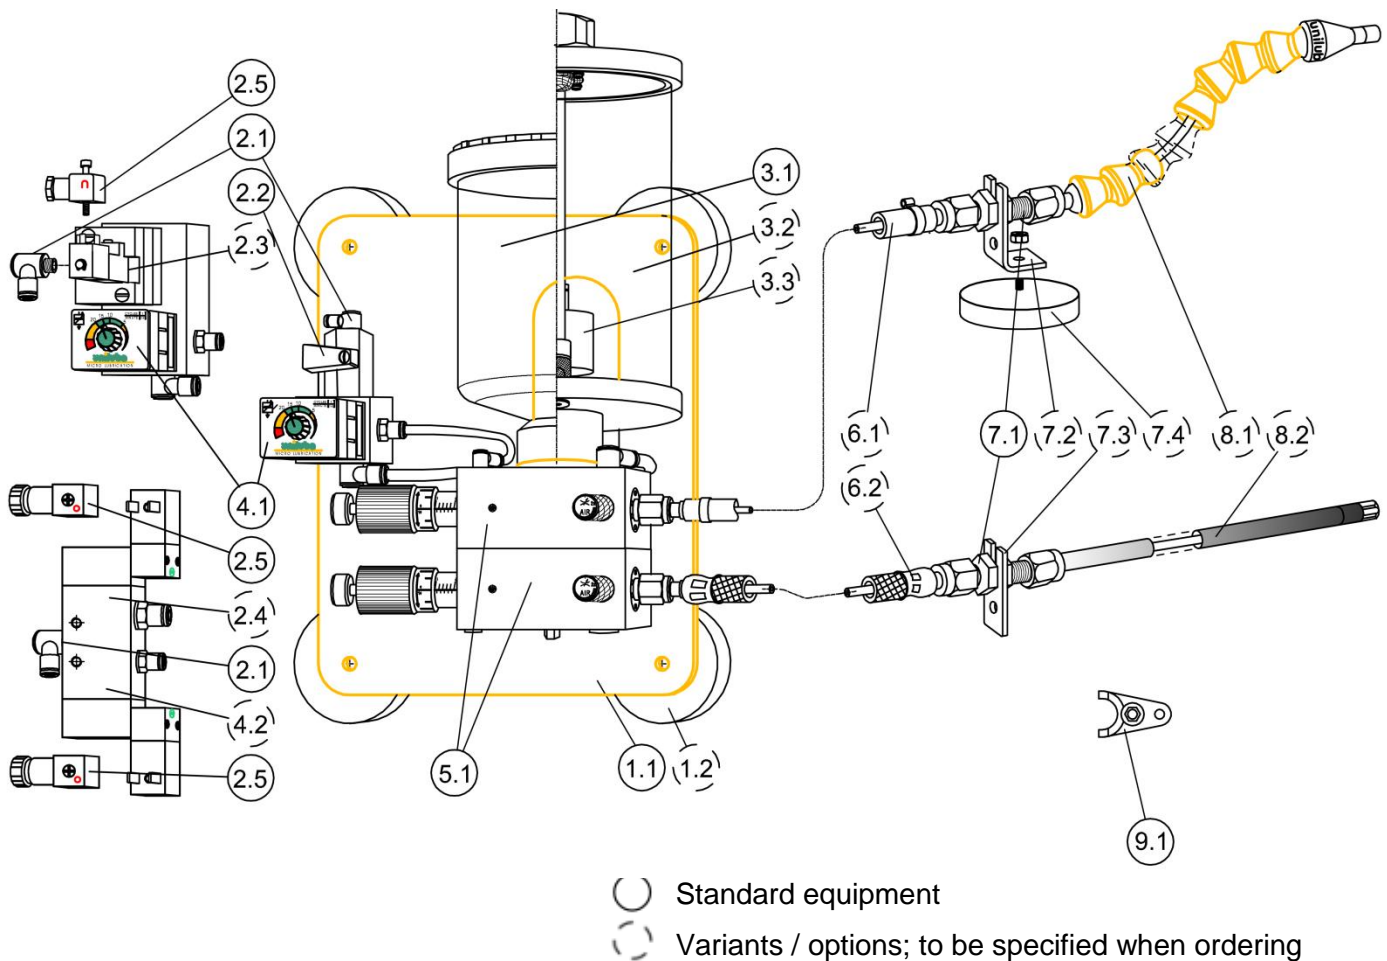


Fig. 2: POPLUBE Minimal Lubrication System

#### 1 Panel

- 1.1 Mounting plate with flange plates (basic dimensions 180 x 230 mm)
- 1.2 Magnetic base plate with rubberised contact surface, 4x Ø43 mm (option)

#### 2 Connections and operation

- 2.1 Compressed-air fitting TUBO Ø 6-4, or G 1/8"
- 2.2 Manual shut-off valve (MSV, 2/2-way, delivered as standard, without option of item 2.3 or 2.4/4.2)
- 2.3 Electric main control valve (MCV, option, instead of item 2.2) only for 1D and 2D
- 2.4 Electric main control valve (MCV, option twinvalve together with item 4.2, instead of item 2.2 or 2.3)
- 2.5 Cable socket with LED power indicator for item 2.2, or 2.3 and 4.2 (size 16x16 mm CI-MIKRO - pin 9.4)

**3 Lubricant system**

- 3.1 Reservoir with screw cap, 0.3 litre version
- 3.2 Reservoir with fine filter and twist lid, 0.8 litre version (option)
- 3.3 Level monitoring (option) with 2-core electric cable (1m)

**4 Metering pump control system**

- 4.1 Pneumatic time relay with control valve (PPG, delivered as standard, without option of item 4.2)
- 4.2 Electric pump control valve (PCV, option twinvalve together with item 2.4, instead of item 4.1)

**5 Lubricant metering**

- 5.1 Combi metering block - initial and follow-up block with integrated metering pump

**6 Coaxial feed line**

- 6.1 Nozzle #1 line (transparent plastic hose variant)
- 6.2 Nozzle #2 line (resistant metal protective hose option)

**7 Nozzle attachment and capillary coupling**

- 7.1 Bulkhead nozzle support (with clamping length  $s \leq 10$  mm)
- 7.2 Retaining bracket (option)
- 7.3 Retaining clamp (option)
- 7.4 Magnetic base plate with rubberised contact surface, Ø43 mm (option)

**8 Coaxial nozzle arm**

- 8.1 Nozzle # 1 (variant with flexible plastic links with aluminium tip)
- 8.2 Nozzle # 2 (variant with rigid stainless steel tube with nozzle head)

**9 Betriebswerkzeug**

- 9.1 Plastic tool for vent screw

## 4. Structure, mounting and connection

- 4.1 The specific structure of the MLS and the components can be seen in the (separate) LAYOUT.
- 4.2 The MLS is fixed vertically to the 4 holes ( $\varnothing$  6.4 mm) of the mounting plate (see LAYOUT). Attachment using 4 magnetic base plates is recommended only when there is a change in use for the workstation.



Fig. 3: POPLUBE Minimal Lubrication System

- 4.3 The MLS must be positioned in such a way that the reservoir is protected from impact – e.g. by foreign parts – (risk e.g. of breakage and leakage) and that the lubricant can be topped up without any risk of spillage.



### Important note:

**Avoid mounting on rapidly accelerating axles as there is a risk of overspill or air entering the hydraulic system**

- 4.4 When installing the coaxial feed line (Fig. 4 consisting of ring line ② with integrated capillary line ①), make sure that neither kinking nor cracking (e.g. over sharp-edged sheet metal) can occur and that the line is not routed through the chip area (risk of destruction). The minimum bending radius of 35 mm (Fig. 4) must be observed. Due to the low weight, the coaxial feed lines should be routed in cable ducts as the top layer where possible.



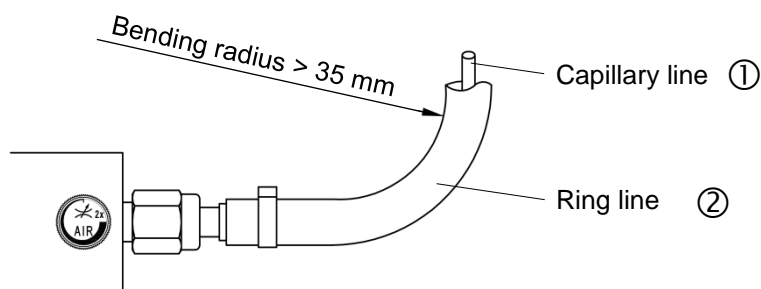


Fig. 4: Coaxial feed line with minimum bending radius



**Important note:**

**Only disconnect the coaxial feed line if absolutely necessary, e.g. to install it in a cable carrier. If possible, only disconnect at the support for the nozzle arm.**

**If the coaxial feed line or the nozzle arm need to be detached more frequently, it is recommended to use the UNILUBE RAPID coax coupling (option).**

- 4.5 The bulkhead nozzle support (Fig. 5 ① M10x1, clamping length  $s \leq 10$  mm) is fixed by the bulkhead nut (Fig. 5 ②) close to the place of use, e.g. in a spindle plate (Fig. 5 ⑤ supplied by the customer) or fastened by means of a retaining clamp (Fig. 5 ③ option) or retaining bracket (Fig. 5 ④ option), so that the nozzle can be oriented in the optimal direction and at the shortest possible distance from the lubrication point or point of need (e.g. at the tool) (see separate TECHNICAL SPECIFICATIONS "Nozzle support" and "Lubricant film application").

A magnetic base plate (option) is only advisable when the place of use changes and must be fitted with good adhesion (risk of the nozzle arm shifting or slipping off).

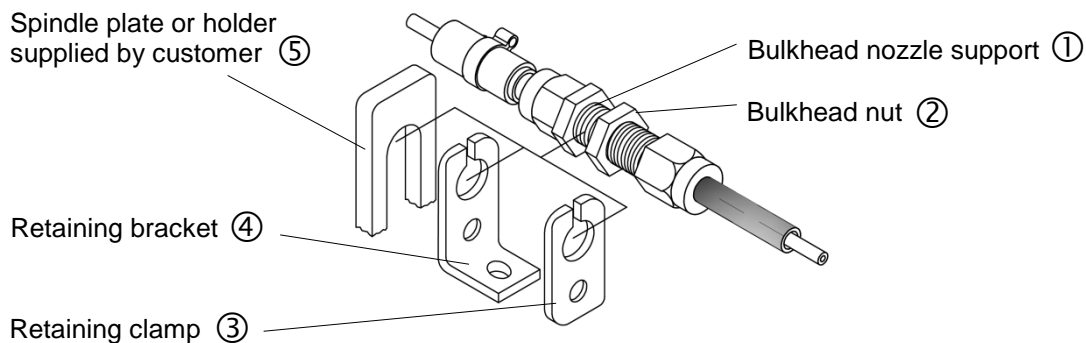


Fig. 5: Bulkhead nozzle support

- 4.6 The compressed-air line is connected via the push-in screw fitting (TUBO Ø 6x4 mm) or the internal thread (G 1/8") of the Manual Shut-off Valve (Fig. 6 ①) or the Main Control Valve

(MCV, Fig. 7 ①, option). When the valve is closed (Fig. 6 ② “Closed” position), the MLS is depressurised; when the valve is open (Fig. 6 ③ “Open” position), compressed air is supplied to the MLS.

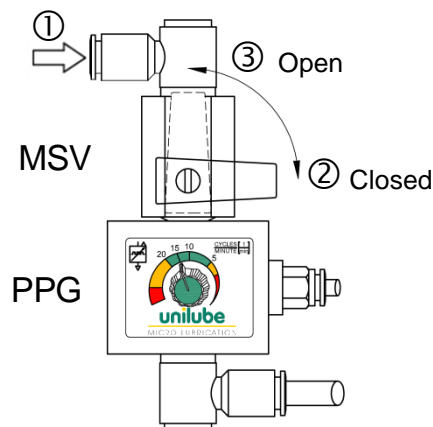


Fig. 6: Manual shut-off valve and Pneumatic Pulse Generator – connection and emergency actuation

The supplied compressed air must be absolutely oil-free and dry (ISO 8573 – class 4), and the required operating pressure must be between a minimum of 5 bar and a maximum of 10 bar; the optimum working range is between 6 and 8 bar.

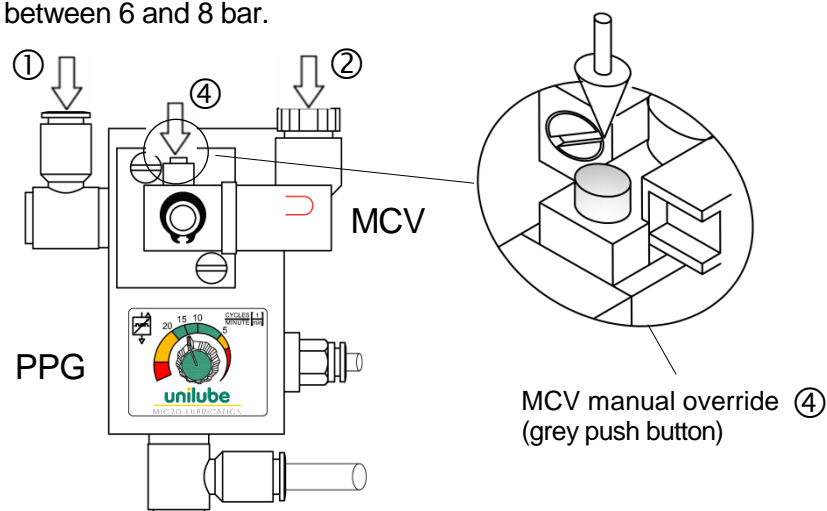


Fig. 7: Electric Main Control Valve and Pneumatic Pulse Generator, connections, LED and manual overrides

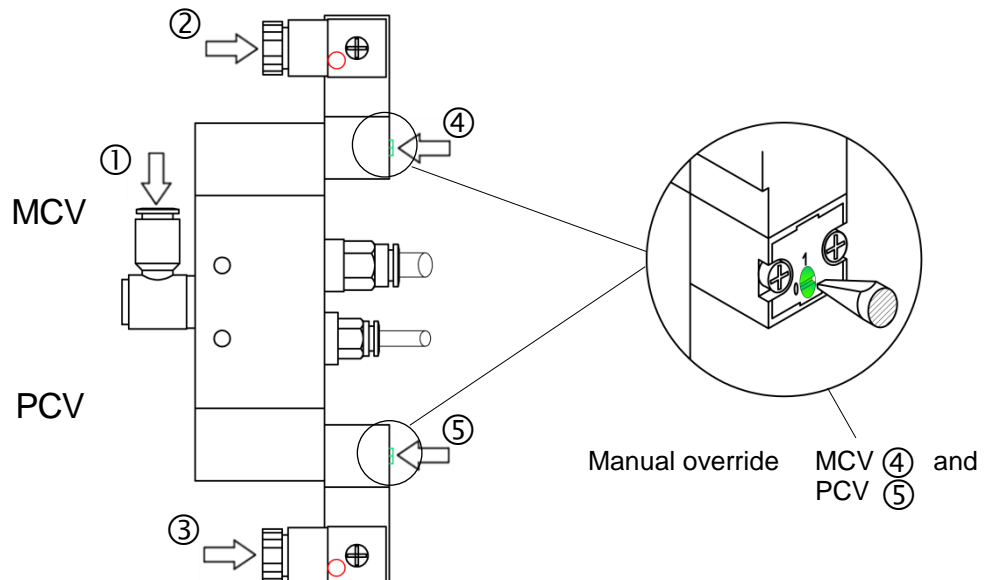


Fig. 8: Twinvalve, Main and Pump Control Valve, connections, LED and manual overrides

If the Manual Shut-off Valve (*Fig. 6 MSV*) is installed, operation (MLS on – MLS of) takes place e.g. via a machine-side control valve. The MSV must be open (*Fig. 6 ③ "Open" position*) for correct function.



**Important note:**

**Before any maintenance work, e.g. on the nozzles, the MLS must be depressurised (electric Main Control Valve switched off on the machine side or Manual Shut-off Valve closed, *Fig. 6 ② "Closed" position*).**

- 4.7 Optional the MLS is coupled to the machine via the electric 3/2-way Main Control Valve with 24 VDC (*Fig. 7 MCV*). A cable socket with LED power indicator (*Fig. 7 ②* or *Fig. 8 ②*) is provided for connection to the machine control system; likewise for connection of the electric Pump Control Valve (option PCV, *Fig. 8 ③*, for setting the delivery cycles, see Chapter 6.4).

When the machine is at a standstill, overrides are provided for maintenance purposes by means of the manual overrides on the electric Main Control Valve via the grey push button (*Fig. 7 ④*) or the screw slot (*Fig. 8 ④*) und am electric Pump Control Valveschen PumpenSteuerVentil über screw slot (*Abb. 8 ⑤*) vorgesehen.



**Important note:**

**Installation may only be carried out by qualified personnel (e.g. industrial electrician)! Before carrying out repairs, the Minimal Lubrication System must be depressurised and de-energised; do not spray or clean it with water.**


## **5. Filling with high-performance lubricant and operating conditions**

- 5.1 Fill the reservoir with **UNILUBE high-performance lubricant** and the MLS is ready for operation (see Chapter 8 "Venting, maintenance and cleaning").


Spilled lubricant must be wiped up immediately.

Dirt particles, e.g. chips or metal dust, must be strictly prevented from entering the reservoir and the hydraulic and pneumatic system (risk of destruction of the micro metering pump).

- 0.3 litre reservoir : Open crew cap (coarse thread and O-ring seal) and place cap separately (*Fig. 9*, beware of contamination with chips)
- 0.8 litre reservoir : Open twist lid (coarse thread and O-ring seal) and place lid on upper flange (*Fig. 10*, protection from loss)

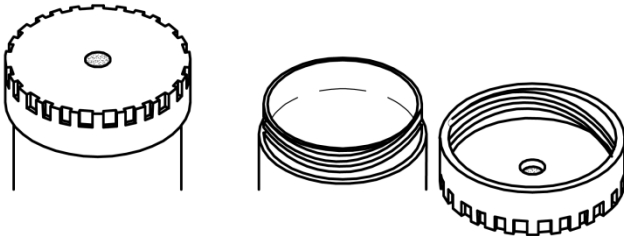

*Fig. 9: 0.3 litre reservoir with screw cap*

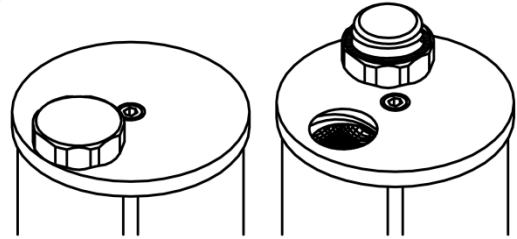

*Fig. 10: 0.8 litre reservoir with twist lid*



**Important note:**

The functionality and efficiency of the Minimal Lubrication System can only be guaranteed when **UNILUBE high-performance lubricants** are used. The safety data sheet and information sheet must be strictly observed.

The use of lubricants from other sources voids all warranties. There is a risk of decomposition (e.g. reservoir glass, seals) or the formation of deposits (e.g. in the metering pump). Furthermore, the composition of the products can result in a loss of performance, with the risk of e.g. tool breakage or workpiece destruction or even a risk of damage to health.

- 5.2 In order to ensure an even application of lubricant, it is recommended, especially after a standstill of longer than 24 hours, to operate the MLS for a few seconds without a consumer (avoid dry running).



**Wichtiger Hinweis:**

**Important note:**

Check the settings of the Minimal Lubrication System at intervals and ensure sufficient ventilation of the working area. Avoid high lubricant concentrations and the formation of oil mist. It is prohibited to use explosive, corrosive or flammable liquids – risk of injury and fire!

## 6. Setting tasks

- 6.1 Setting the metering quantity: The metering pump meters the lubricant precisely and at high pressure. The piston stroke and thus the delivery rate can be steplessly varied by turning the micrometer screw (Fig. 11 ①), the total adjustment range being 5 turns and the POPLUBE-metering pump has a minimum delivery rate at 0 (see Fig. 20).



### Important note:

**Adjust the micrometer screw gradually and not beyond the two end stops (minimum and maximum) (risk of destroying the metering pump).**

The set values can be read off precisely from the two scales on the micrometer screw (Fig. 11 ② and ③) each mark on the scale representing a 2% change in the piston stroke. Experience has shown that the optimum working range is between 0.1 and 0.5 turns (corresponding to 11% and 14.5% delivery rate, see Fig. 20).


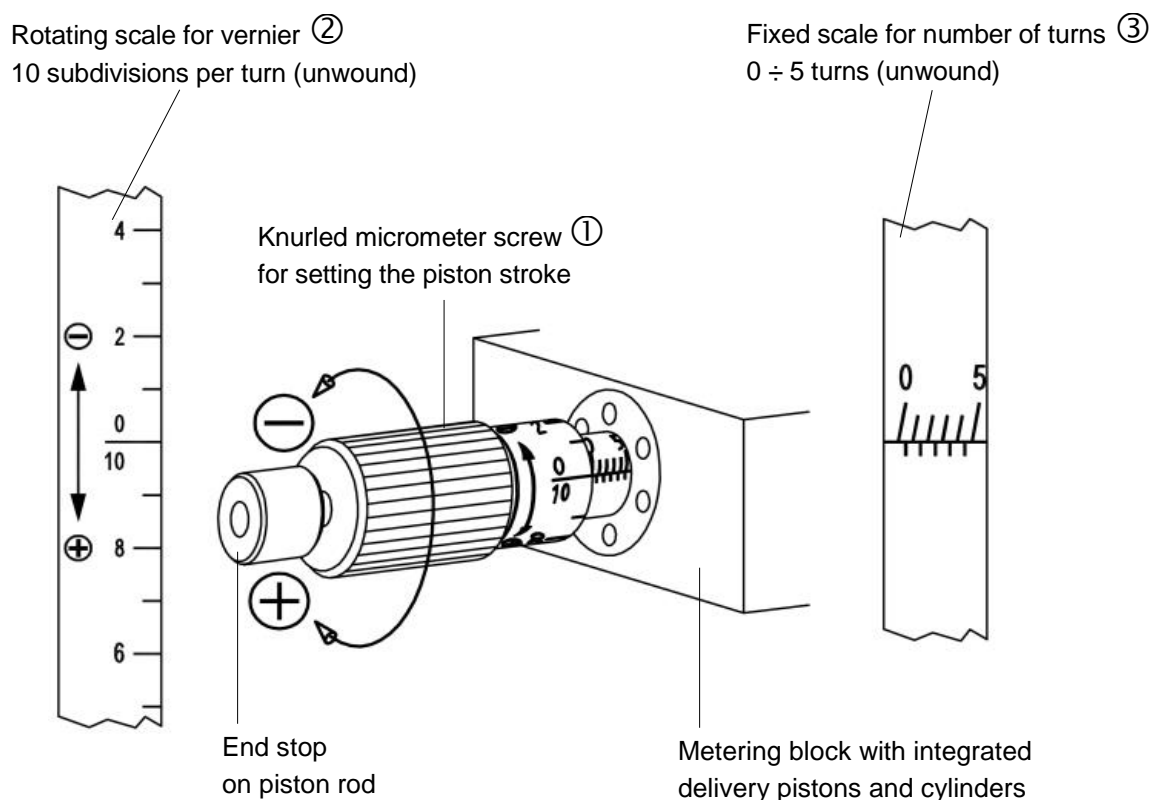


Fig. 11: Metering pump – regulating knob, metering stroke setting with micrometer display for stepless adjustment 0 ÷ 5 turns (10 ÷ 100% delivery rate)

- 6.2 The function of the Minimum Lubrication System and especially of the nozzles can be checked and visualised e.g. with a paper strip or ideally with a plastic disc. These are moved past the nozzle tip at a distance of about 10 mm. The applied lubricant leaves a fine and even pattern – corresponding to the delivery setting selected – without any drops being formed. This check should be done at regular intervals.

A perfect micro-film of lubricant is visible by eye on the plastic disc when held up to the light.

- 6.3 Setting the number of cycles: The Pneumatic Pulse Generator (PPG *Fig. 6, 7 & 14*) determines the cycling of the metering pump; the setting is steplessly variable from 0 to approx. 60 pulses/minute by turning the toggle knob (optimum working range: 5 ÷ 20 pulses/minute, *Fig. Abb. 15* green). The adjustment range has no stop and the toggle knob can be turned in either direction as desired.

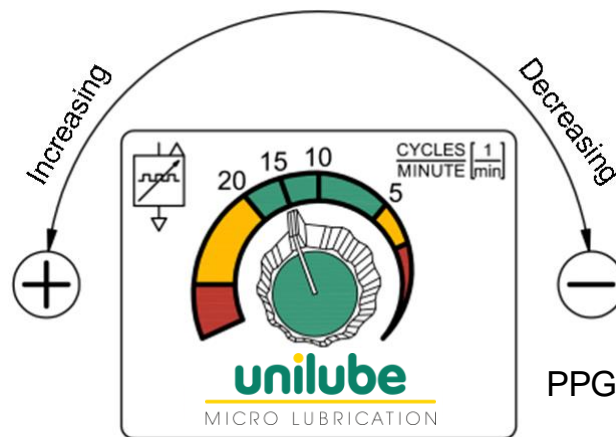

*Fig. 12: Pneumatic Pulse Generator – setting number of cycles (5 ÷ 20 pulses/min)*

When the electric Pump Control Valve (PCV option, *Fig. 8*) is used, the cycling of the metering pump is determined via the machine control system. With a fixed switch-on time (approx. 0.5 seconds), the quantity of lubricant required for the respective process is set by varying the switch-off time (see separate CONTROL DIAGRAM "Minimal Lubrication System with programmable delivery rate").


- 6.4 When using the MLS as an "air nozzle" without the application of high-performance lubricant, it should be noted that:

By reducing the number of cycles to 0 (see Chapter 6.3), the effect of pure air delivery is achieved. Here and with subsequent reuse of the MLS with **UNILUBE high-performance lubricant**, run-in phases (with no consumer) are necessary to achieve constant conditions:



- For operation with pure air : The run-in phase discharges lubricant residues from the nozzle.
- For operation with lubricant : After the run-in phase, dry running (lack of microlubrication) is prevented by a constant discharge of lubricant.

6.5 Mixing air setting: The mixing air creates a microfine film of lubricant from the droplet particles and influences the degree of aerosol formation with a mixing ratio of lubricant to air of about 1 : > 1 million, as well as chip removal, etc. Each nozzle is set individually using the associated knurled knob (*Fig. 13*, labelled "AIR"). The adjustment range has an almost linear characteristic curve and is limited to 2 turns (max. 100 NI/min per nozzle at 6 bar operating pressure). The optimal working range when using the standard nozzle is between 0.5 and 1.5 turns.

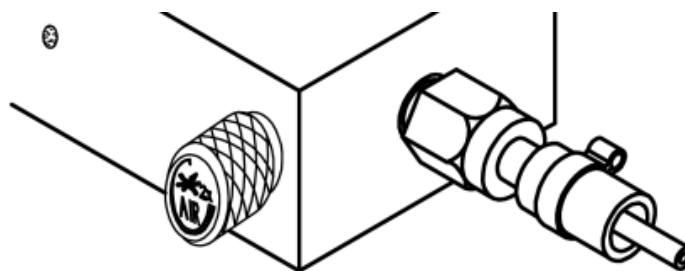

*Fig. 13: Regulating knob with knurled knob – flow rate of mixing air*

## 7. Factory settings

7.1 After testing, the Minimal Lubrication System is delivered with the following factory settings:

### 7.1.1 Piston stroke of the metering pump

Micrometer screw turned up 0.5 turns  
( $\hat{=}$  14.5 % delivery rate, *Fig. 11*)



*Fig. 14: Micrometer screw – factory setting 0.5 turns*

### 7.1.2 Number of cycles


- Version with Pneumatic Pulse Generator  
15 pulses/minute ( $\hat{=}$  15 piston strokes/min, *Fig. 6*)



*Fig. 15: Pneumatic Pulse Generator – factory setting 15 cycles / min*

- Version with electric Pump Control Valve

Programmed pulses ( $\hat{=}$  CNC machine control system *Fig. 8*)  
(depends on what the customer has programmed)



*Fig. 16: Electric Pump Control Valve – cycles from control system*

### 7.1.3 Mixing air

Knurled knob opened by 1.0 turn  
( $\hat{=}$  50 NI/min, *Fig. 13*)



*Fig. 17: Air regulation – factory setting open by 1 turn*

The setting data listed above apply as general guide values for many applications using **UNILUBE high-performance lubricants**. However, each use case requires individual adjustment to the conditions; experience has shown that the delivery rate of the metering pump can still be significantly reduced under optimised operating conditions (see Chapter 10 "Lubricant consumption values").



**Important note:**

**Check the settings of the Minimal Lubrication System at intervals and ensure sufficient ventilation of the working area. Avoid high lubricant concentrations and the formation of oil mist. It is prohibited to use explosive, corrosive or flammable liquids – risk of injury and fire!**

## 8. Venting, maintenance and cleaning

- 8.1 Before starting up for the first time and after any maintenance work on the coaxial line or nozzle, the MLS must be vented. As long as the quantity of high-performance lubricant in the reservoir does not fall below a minimum level (intake opening covered, fine filter), no further venting is usually necessary.

A level monitoring system (*Fig. 2 item 3.3 & Fig. 3*, option for reservoirs with a nominal volume of 0.8 litres), which can be supplied separately, prevents unintentional emptying because a

signal has been emitted prematurely (refer to separate TECHNICAL SPECIFICATION "Level monitoring").

8.2 The Minimal Lubrication System is vented as follows:

8.2.1 Fill the reservoir with **UNILUBE high-performance lubricant** (Chapter 5.1) and do not close the lid during the venting phase to ensure unobstructed air equalisation.

8.2.2 Open the vent screw (Fig. 18 ①) on the underside of the metering block by hand or with the service tool (Fig. 18 ② SW 6.35) by approx. 2 turns and drain the lubricant until it comes out without any bubbles (duration: approx. 5 seconds); then close it fully again. Tightening by hand is sufficient (O-ring locking). To flush out the hydraulic system or to empty the reservoir, the vent screw can be unscrewed completely.

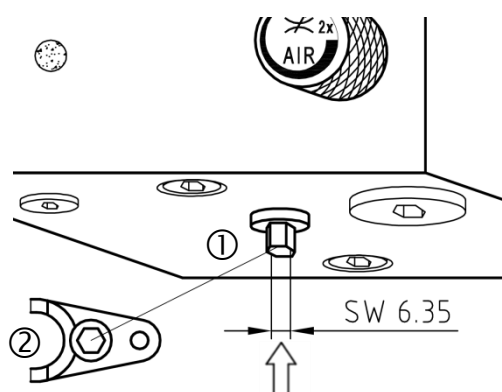


Fig. 18: Vent screw ① on underside of metering block – tool ② with hex socket

8.2.3 Increase the piston stroke of the metering pump to its maximum (open by 5 turns Fig. 11 ① and Chapter 6.1).

8.2.4 Increase the number of cycles of the PPG to approx. 60 (-120) pulses/minute (Fig. 12 and Chapter 6.3). For versions with an electric Pump Control Valve (option) in the machine control system, select the setting for venting (depends on what the customer has programmed).

8.2.5 Reduce the air volume of the nozzle via the air regulating screw (Fig. 13) to 0.5 turns.

8.2.6 Operate the piston rod by hand. To do this, press the end stop of the micro metering pump (Fig. 11) against the micrometer screw approx. 10 times. With no lubricant in the capillary line (Fig. 19 ① inner pressure hose of the coaxial feed line), lubricant can be seen to enter the capillary line after approx. 8 strokes and air is removed from the hydraulic system.

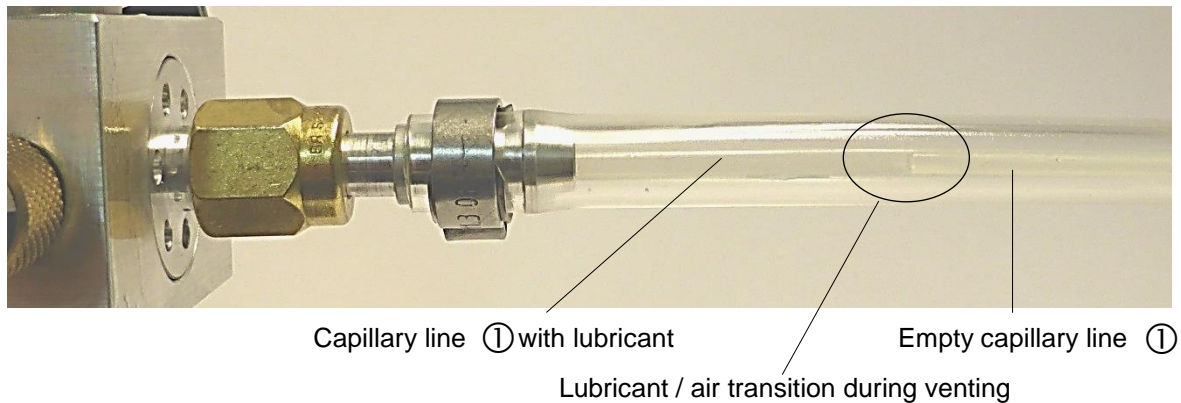


Fig. 19: Capillary line ① filling with lubricant during venting

8.2.7 Switch on the compressed air (e.g. by overriding the MCV Fig. 7 or Fig. 8 ④) and watch the air bubbles move through the capillary line until the line is free of bubbles over its entire length up to the nozzle head (duration: approx. 0.75 minutes / 1 metre coax line length).

8.2.8 After the venting process is complete, restore the piston stroke, number of cycles and air volume to the operating values (Chapter 7) and fully close the reservoir.

8.2.9 The functioning of the Minimal Lubrication System and especially of the nozzles can be checked and visualised e.g. with a paper strip or ideally with a plastic disc. These are moved past the nozzle tip at a distance of about 10 mm. The applied lubricant leaves a fine and even pattern corresponding to the delivery setting selected. This check should be done at regular intervals.

8.3 Each time before the reservoir is filled with **UNILUBE high-performance lubricant**, check the Minimal Lubrication System for leaks or defects; if necessary, remove dirt, chips, etc. with a neutral cleaning agent.



**Important note:**

**When working on the nozzles, make absolutely sure that the tools are at a standstill and the machine is switched off; for maintenance purposes, simulate operation with manual override (see Fig. 7 or Fig. 8 ④ and Chapter 4.7). Do not point the nozzle tip at people, especially not at their eyes – risk of injury!**

## 9. Quick start-up guide



- 9.1 Mount the MLS, fix the lines and nozzles, connect the MLS electrically and pneumatically  
Detail: Chapter 4
- 9.2 Fill reservoir with UNILUBE high-performance lubricant  
Detail: Chapter 5.1
- 9.3 Open the drain and vent screw until lubricant is discharged without any bubbles, then close it  
Detail: Chapter 8.2.2
- 9.4 Turn up the delivery rate of the metering pump to its maximum (5 turns) using the micrometer screw  
Detail: Chapter 8.2.3
- 9.5 Set the PPG to approx. 90 pulses/min or the setting in the machine control system for PCV to vent and set the air regulating screw to approx. 0.5 turns  
Detail: Chapter 8.2.4 and 8.2.5
- 9.6 Operate the metering pump manually until lubricant / bubbles can be seen to move in the capillary line  
Detail: Chapter 8.2.6
- 9.7 Operate the MLS mechanically or electrically  
Detail: Chapter 4.7 & 8.2.7
- 9.8 Shut off the MLS mechanically or electrically when the capillary line has no air bubbles in it
- 9.9 Set factory settings or individual required values (metering pump, air regulating screw, Pneumatic Pulse Generator or Pump Control Valve)  
Detail: Chapter 7

## 10. ECOLUBE "μ" consumption values

10.1 The following diagrams (*Fig. 20 & 21*) and calculations allow the lubricant consumption to be determined for different settings. The values are based on continuous operation; when coupled with the work process (e.g. feed rate), reductions in consumption of 50% or more can be achieved. The settings are made according to Chapter 7.

10.2 Example with "factory setting" (heavy chip removal):

Consumption with 0.5 turns of micrometer screw and 20 pulses/minute (*Fig. 20 & 21*)

Calculation:

Maximum delivery rate		0.0375 ml/stroke	(100 % piston stroke of metering pump)
Minimum delivery rate	-	0.0038 ml/stroke	(Minimum piston stroke at 0 = minimum turn)
Piston stroke setting	x	0.1	(10 % delivery rate = 0.5 turns)
Minimum delivery rate	+	0.0038 ml/stroke	(Minimum piston stroke at 0 = minimum turn)
Setting for number of cycles	x	15 pulses/min	(15 strokes of metering pump)
Operating time	x	60 min	(1 hour)

Consumption per process hour = **6.45 ml/h** (continuous operation with "Factory setting")

10.3 Example with "HSC machining" (light machining):

Consumption with 0.2 turns of micrometer screw and 10 pulses/minute (*Fig. 20 & 21*)

Calculation:

Maximum delivery rate		0.0375 ml/Hub	(100 % piston stroke of metering pump)
Minimum delivery rate	-	0.0038 ml/Hub	(Minimum piston stroke at 0 = minimum turn)
Piston stroke setting	x	0.04	(4 % Förderleistung = 0.2 Umdrehung)
Minimum delivery rate	+	0.0038 ml/Hub	(Minimum piston stroke at 0 = minimum turn)
Setting for number of cycles	x	10 Imp/min	(10 strokes of metering pump)
Operating time	x	60 min	(1 hour)

Consumption per process hour = **3.09 ml/h** continuous operation with "HSC machining")



**Important note:**

The Minimum Lubrication System is delivered with the factory settings according to Chapter 7. The parameters required for individual use cases depend on various factors (e.g. the process, material, tool) and must be optimised individually during operation.



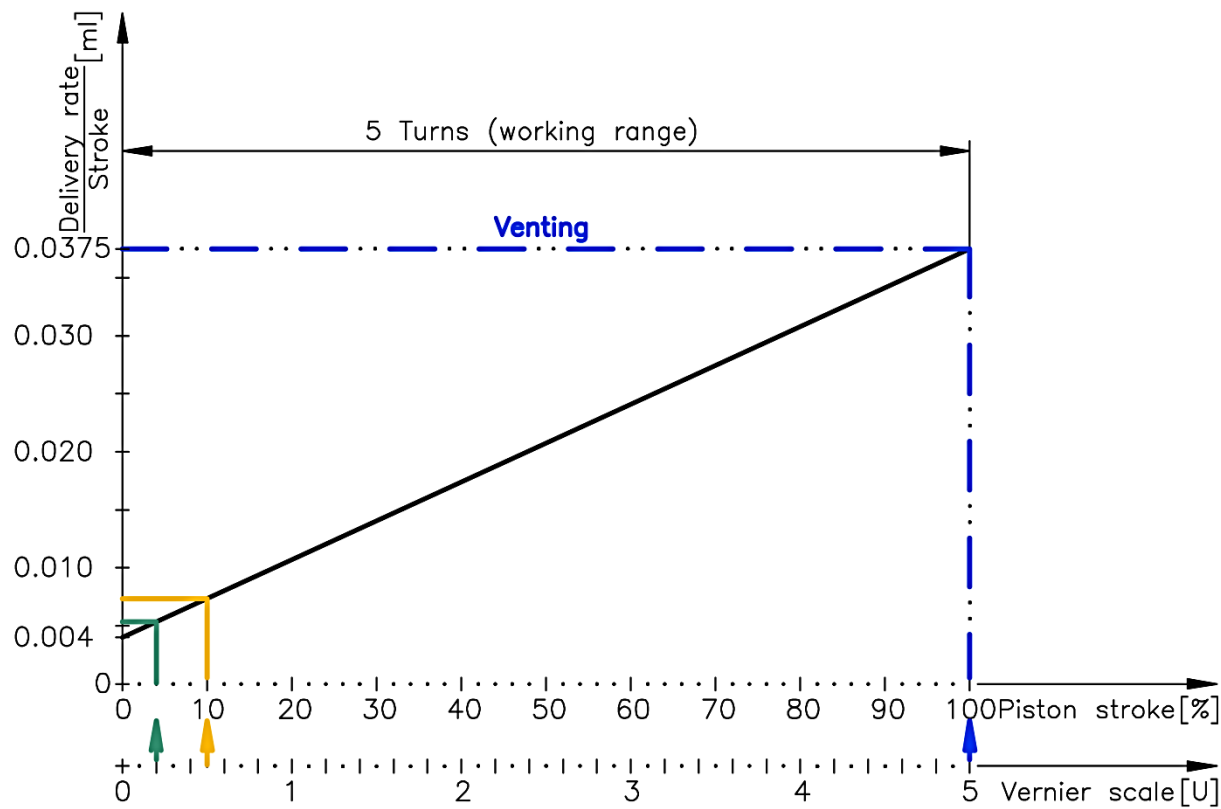


Fig. 20: Delivery rate as a function of the piston stroke

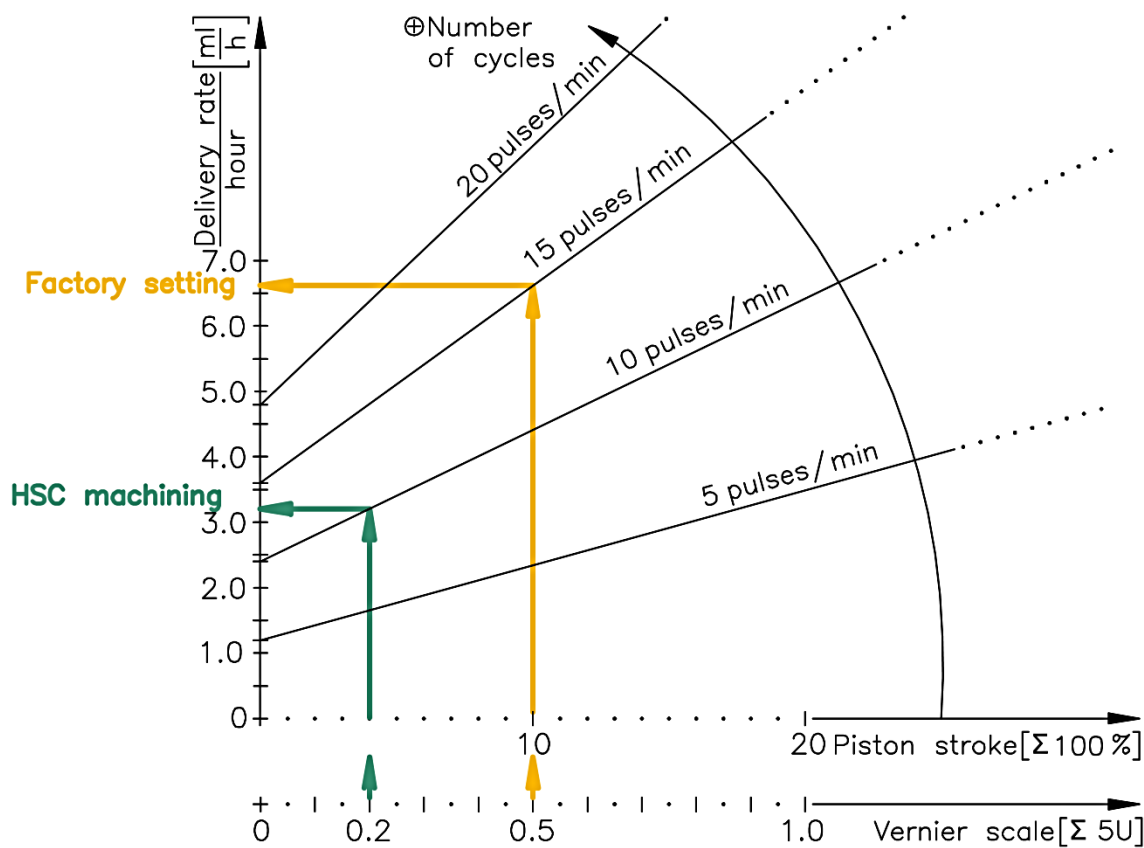


Fig. 21: Consumption as a function of the piston stroke and at different cycle rates (pulses/min)

## 11. Supplementary documentation

### 11.1 Available on request:

	Document number
Layout: POPLUBE 1D, 2D, 3D .....	SP 9262
Technical specification: main control valve .....	TS 3037
Technical specification: Twin valve .....	TS 3048
Control diagram: MLS with programmable delivery rate .....	SP 9093
Technical specification: level monitoring .....	TS 3011
Nozzle support: design variants .....	SP 9107
Technical specification: universal nozzle support .....	TS 3010
Technical specification: RAPID coax coupling .....	TS 3046
Technical specification: coax standard nozzle .....	TS 3024
Mounting recommendation: nozzles oriented at saw blade 1D, 2D, 3D ....	SP 9157
Technical specification: Flexline coax nozzle .....	TS 3047
Technical specification: spray patterns .....	TS 3013
Technical specification: circular saw support .....	TS 3040
Technical specification: band saw support .....	TS 3023
Project outline: ring nozzle .....	SP 9271
Technical specification: TIMJET .....	TS 3038
UNILUBE 2032 safety data sheet .....	TS 3029
UNILUBE 9107 safety data sheet .....	TS 3030
Information sheet on UNILUBE high-performance lubricants .....	TS 3036

### 11.2 Further drawings of applications and projects available on request.

## 12. Verwendete Abkürzungen

MSV	Manual shut-off valve
MCV	Main control valve
ISO	International Organization for Standardization
LED	Light-emitting diode
KoAx	Koaxial (z.B. Düsenarm, Zuführleitung)
MSS	Minimum Lubrication System
NBR	Nitrile butadiene rubber
PA	Polyamide
PPG	Pneumatic pulse generator
PU	Polyurethane
PCV	Pump control valve
TIM(JET)	Tool Integrated microlubrication
VDC	Volts of direct current

